



EUROPEAN PATENT APPLICATION

(12)

(43) Date of publication:
03.04.2002 Bulletin 2002/14

(51) Int Cl.7: **G01R 33/38**

(21) Application number: **01308414.0**

(22) Date of filing: **02.10.2001**

(84) Designated Contracting States:
AT BE CH CY DE DK ES FI FR GB GR IE IT LI LU
MC NL PT SE TR
 Designated Extension States:
AL LT LV MK RO SI

(30) Priority: **02.10.2000 US 676945**

(71) Applicant: **GENERAL ELECTRIC COMPANY**
Schenectady, NY 12345 (US)

(72) Inventors:
 • Edelstein, William Alan
 Schenectady, New York 12309 (US)
 • Mallozzi, Richard Philip
 Clifton Park, New York 12065 (US)
 • Hedeon, Robert Arvin
 Clifton Park, New York 12065 (US)
 • El-Hamamsy
 Niskayuna, New York 12309 (US)
 • Miller, Mark Lloyd
 Schenectady, New York 12309 (US)
 • Thompson, Paul Shadforth
 Stephentown, New York 12168 (US)

- Ackermann, Robert Adolph
 Schenectady, New York 12304 (US)
- Amm, Bruce Campbell
 Clifton Park, New York 12065 (US)
- Fura, John Peter
 Ballston Lake, New York 12019 (US)
- Radziun, Mike James
 Waterford, Wisconsin 53185 (US)
- Dean, David Edward
 Hartland, Wisconsin 53185 (US)
- Mansell, Scott Thomas
 Waterford, Wisconsin 53185 (US)
- Purgil, Dewain Anthony
 Waukesha, Wisconsin 53188 (US)
- Vavrek, Robert Michael
 Waukesha, Wisconsin 53188 (US)

(74) Representative: **Goode, Ian Roy**
GE LONDON PATENT OPERATION,
Essex House,
12/13 Essex Street
London WC2R 3AA (GB)

(54) **Low noise MRI scanner**

(57) A low noise imaging apparatus for producing Magnetic Resonance (MR) images of a subject and for substantially minimizing acoustic noise generated during imaging is provided. The imaging apparatus comprises a magnet assembly (4,6,7), a gradient coil assembly (3), and a rf coil assembly (2), wherein at least one of the magnet assembly, the gradient coil assembly and the rf coil assembly are configured to reduce the generation and transmission of acoustic noise.

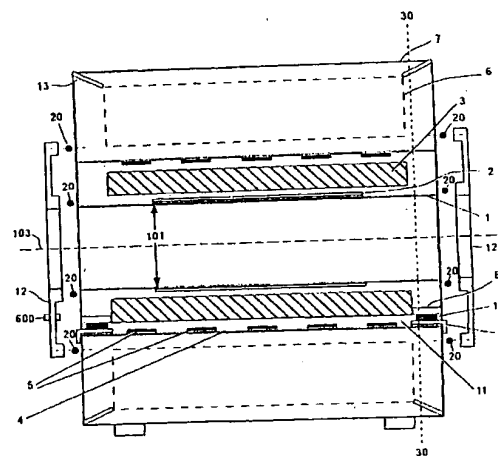


Fig. 1

Description

[0001] The present invention relates generally to a magnetic resonance imaging (MRI) scanner and more particularly to a low-noise MRI scanner.

[0002] MRI scanners, which are used in various fields such as medical diagnostics, typically use a computer to create images based on the operation of a magnet, a gradient coil assembly, and a radiofrequency coil(s). The magnet creates a uniform main magnetic field that makes nuclei, such as hydrogen atomic nuclei, responsive to radiofrequency excitation. The gradient coil assembly imposes a series of pulsed, spatial-gradient magnetic fields upon the main magnetic field to give each point in the imaging volume a spatial identity corresponding to its unique set of magnetic fields during the imaging pulse sequence. The radiofrequency coil creates an excitation frequency pulse that temporarily creates an oscillating transverse magnetization which is detected by the radiofrequency coil and used by the computer to create the image. Typically, there is a radiofrequency coil and a gradient coil assembly within the magnet.

[0003] Magnets for MRI scanners include superconductive-coil magnets, resistive-coil magnets, and permanent magnets. Known superconductive magnets include liquid-helium cooled and cryocooler-cooled superconductive magnets. Known superconductive magnet designs include cylindrical magnets and open magnets.

[0004] Cylindrical magnets typically are cylindrically shaped and have an axially-directed static magnetic field. In MRI systems based on cylindrical magnets, the radiofrequency coil, the gradient coil assembly and the magnet are generally annularly-cylindrical shaped and are generally coaxially aligned, wherein the gradient coil assembly circumferentially surrounds the radiofrequency coil and wherein the magnet circumferentially surrounds the gradient coil assembly.

[0005] Open magnets typically employ two spaced-apart magnetic assemblies with the space between the assemblies allowing for access by medical personnel for surgery or other medical procedures during MRI imaging. The open space helps the patient overcome feelings of claustrophobia that may be experienced in a cylindrical magnet design.

[0006] Generally, the various components of the MRI scanner represent sources and pathways of acoustic noise that can be objectionable to the patient being imaged and to the user of the scanner. For example, the gradient coil assemblies of MRI scanners generate loud acoustic noises which many medical patients find objectionable. The acoustic noises occur internal to the patient bore of the scanner as well as outside of the scanner. Active noise control techniques have been used to reduce gradient coil assembly noise including noise-canceling patient earphones. Known passive noise control techniques include locating the gradient coil assembly

bly in a vacuum enclosure.

[0007] The rf coil structure is also another source of vibration and acoustic noise. An MRI system employs electrically excited gradient coils to impose time varying magnetic fields on the primary or B_0 magnetic field. These time varying fields tend to induce eddy currents in the conductors of the rf coil, which in turn may cause mechanical motion of the rf coil.

[0008] Yet another source and pathway of acoustic noise is due to vibration of mechanical components in the scanner. It is known in the mechanical arts area to design and use isolation mounts so that vibrations from machinery supported by the isolation mounts are not transmitted to surrounding structure that supports the isolation mounts. Conventional isolation mounts include those of the elastomeric type and those of the spring type. Such isolation mounts are designed by the artisan so that the natural frequency of vibration of the mounts and the machinery is less than the important excitation frequencies of the machinery in order to provide effective vibration isolation.

[0009] These techniques or measures to reduce acoustic noise due to the various components in the MRI scanner have been partially effective, but patients and technicians still find the noise in and about a MRI scanner to be problematic. What is needed is a lower noise MRI scanner that addresses the multiple sources and pathways of acoustic noise in and about the scanner.

[0010] According to the invention, there is provided a low noise imaging apparatus for producing Magnetic Resonance (MR) images of a subject and for substantially minimizing acoustic noise generated during imaging is provided. The imaging apparatus comprises a magnet assembly, a gradient coil assembly, and a rf coil assembly, wherein at least one of the magnet assembly, the gradient coil assembly and the rf coil assembly are configured to reduce the generation and transmission of acoustic noise in and about the imaging apparatus.

[0011] The invention also provides a radio frequency (rf) coil assembly for a Magnetic Resonance Imaging (MRI) system comprises a plurality of conductors wherein each of the conductors has a width selected for transmitting a radiofrequency pulse, for receiving an MR signal induced in the subject and for reducing eddy current excitation contributing to acoustic noise in and about the imaging apparatus. Further, a layer of acoustic absorptive material may be disposed between the plurality of conductors and a patient bore tube.

[0012] A magnet assembly for an imaging apparatus for a Magnetic Resonance Imaging (MRI) system comprises an outer surface and a plurality of suspension members for attaching a magnet to the outer surface. The suspension members are configured to reduce generation and transmission of acoustic noise.

[0013] The features and advantages of the present invention will become apparent from the following detailed description of the invention when read with the accompanying drawings in which:

Figure 1 is a schematic cross-sectional side-elevation view of an imaging apparatus to which preferred embodiments of the present invention are applicable;

Figure 2 is a schematic cross-sectional view of the imaging apparatus of Figure 1 taken along the line 30 - 30 of Figure 1;

Figure 3 is a schematic cross-sectional side-elevation view of a MRI scanner to which preferred embodiments of the present invention are applicable;

Figure 4 is a schematic illustration of a rf coil assembly of a type useful in the imaging apparatus of Figures 1 and 3;

Figure 5 is a schematic illustration of a rf coil assembly of a type useful in the imaging apparatus of Figures 1 and 3; and,

Figure 6 is a schematic illustration of a gradient current feed-through arrangement of a type useful in the imaging apparatus of Figures 1 and 3.

[0014] Referring to Figures 1, 2 and 3, there is shown an exemplary imaging apparatus to which embodiments of the present invention are applicable. The imaging apparatus is of a type useful in producing Magnetic Resonance (MR) images of a patient or subject. Throughout the figures, like numerals represent like elements throughout. Figures 1, 2 and 3 show a MR system based on a cylindrical superconducting magnet. It is to be appreciated by one skilled in the art that the functions and descriptions of similar components used in an open magnet configuration are applicable for an open magnet MR system.

[0015] Referring to Figure 2, a cross-sectional view of a magnet arrangement of a type commonly used in connection with MR imaging is shown. A magnet assembly is generally cylindrical and annular in shape, and comprises an inner surface referred to as a magnet warm bore 4, passive magnet shims 5 (also shown in Figure 1), magnet vessel 6 and cryostat shell 7 disposed radially around the outer surface. The magnet assembly further comprises suspension members 13 and end cap seals 20 which will later be described in more detail.

[0016] Typically, magnet vessel 6 encloses a superconductive magnet (not shown) that, as is well-known, includes several radially-aligned and longitudinally spaced-apart superconductive main coils, each capable of carrying a large, identical electric current in the same direction. Also, the superconductive main coils are designed to create a magnetic field of high uniformity within a spherical imaging volume centered within the magnet's bore where the object to be imaged is placed. The superconductive main coils produce a main static magnetic field, known as B_0 , typically in the range from 0.5

T to 8 T. The superconductive main coil is enclosed by magnet vessel 6. Magnet vessel 6 generally includes a helium vessel and thermal or cold shields for containing and cooling the magnet windings in a known manner.

Magnet vessel 6 also prevents heat from being transferred to the superconducting magnet. Hereinafter, magnet vessel 6 refers generally to the superconductive main coils described herein, conventional thermal shields, liquid-helium dewars, and the like, being omitted from the figures for clarity. Cryostat shell 7 covers the outer surface of the magnet assembly. Cryostat shell 7 is generally metallic, typically steel or stainless steel.

[0017] Referring further to Figure 2, rf coil assembly 2, gradient coil assembly 3 and the magnet assembly are generally annularly-cylindrical shaped and are generally coaxially aligned, wherein the gradient coil assembly circumferentially surrounds the radiofrequency coil and wherein the magnet circumferentially surrounds the gradient coil assembly. Referring to Figure 1, a side-elevation view shows the relative placement of each of the components of the imaging apparatus. A patient or imaging subject 200 (not shown, see Figure 3) is positioned within a cylindrical imaging volume 101 surrounded by patient bore tube 1. Patient or subject 200 is inserted into the imaging apparatus along center axis 103 on a patient table or cradle 104 (not shown, see Figure 3). Center axis 103 is aligned along the axis of the magnet assembly parallel to the direction of the B_0 magnetic field. Bore tube 1 is desirably made of electrically low- or non-conducting material such as FRP (fiberglass-reinforced plastic). In this embodiment, rf coil assembly 2 is mounted on the outer surface of patient bore tube 1, such as in a conventional birdcage rf coil arrangement, e.g. multiple conductors and capacitive elements spaced apart along outer surface the patient bore tube in order to maintain a uniform radiofrequency (rf) magnetic field. Rf coil assembly 2 is used to apply a radiofrequency magnetic field pulse to patient or subject 200 and to receive MRI information back from subject 200, as is well-known in the art of MR imaging. Gradient coil assembly 3 is disposed around in a spaced apart coaxial relationship therewith and generates time-dependent gradient magnetic field pulses in a known manner. Radially disposed around gradient coil assembly 3 is the magnet assembly including warm bore 4, magnet vessel 6 and cryostat shell 7 that produces the static magnetic field necessary for producing MRI images, as described above.

[0018] Referring further to Figure 1, warm bore 4 refers generally to the inner cylindrical surface of the magnet assembly. This magnet warm bore is typically made of metal. On the inside cylindrical surface of warm bore 4 are passive magnetic shims 5. Shims 5 are used in a well-known manner to make small adjustments to the static magnetic field. The shims are typically thin iron or steel strips.

[0019] Referring further to Figure 1, the imaging apparatus further comprises a pair of end caps 12 for en-

closing the components of the imaging apparatus. End caps 12 hold the patient bore tube 1 in place by fixably attaching end portions of patient bore tube 1 to the magnet assembly. End cap seals 20 act as an airtight seal between end caps 12 and patient bore tube 1, and also maintain vacuum space 11 for enclosing gradient coil assembly 3. End cap seals 20 are typically made of compliant gasket material having a thickness between $\frac{3}{4}$ - 1 inch in order to maintain the desired vacuum in vacuum space 11. End cap seals 20 have their elastic properties selected so that they can provide vibration isolation between the magnet cryostat shell 7 and the end caps 12.

[0020] Referring to Figure 3, further components of the imaging apparatus include support structures such as patient couch or cradle 104 in order to insert and position subject 200 into imaging volume 101. Patient cradle 104 is slidable, such as with rollers, in a known manner along bridge 102. Bridge 102 is supported by front bridge support 105 and rear bridge support 106. Each bridge support is fixed to the floor or the magnet assembly. Further, cradle electronics unit is coupled to bridge 102 or cradle 104 to control motion of patient cradle 104.

[0021] Gradient coil assembly 3 generally contributes two sources of acoustic noise in an MR imaging system - 1) vibrations due to Lorentz (electromagnetic) forces acting on the gradient coils and 2) noise due to Lorentz forces in electrically conductive parts not in contact with the gradient coil assembly. Gradient coil assembly 3 comprises gradient windings that are typically wires or flat conducting strips shaped into forms that produce desired gradient magnetic fields. The gradient winding wires are in a strong magnetic field and therefore experience a Lorentz force $\propto \vec{I} \times \vec{B}$, where \vec{I} is the current in any section of wire and \vec{B} is the static magnetic field. Further, the currents in the wires are typically as high as several hundred Amps and the static magnetic fields can vary from typically 0.5 T to 8 T. Therefore, the Lorentz forces can be very large and produce significant vibrations of the gradient assembly. These vibrations can in turn displace air and produce audible sound. The gradient assembly vibrations can also be transmitted mechanically through the magnet system structures and can cause vibrations in other parts of the structure and subsequent sound generation. The second source of acoustic noise is generated by Lorentz forces in electrically conductive parts not in contact with the gradient assembly. For example, these forces are produced because the gradient pulsed fields induce eddy currents in various electrically conductive parts of the MRI system, and these eddy currents interact with the static magnetic field to produce $\vec{I} \times \vec{B}$ Lorentz forces as described above.

[0022] The rf coil assembly is also a source of acoustic noise in an MR imaging system. Rf coil assembly 2 typically is a large-volume rf coil, mounted in a bird cage configuration, and is made using etched patterns of conductors, and these conductors can typically be a few inches wide. A large-volume rf coil is typically about half

the length of the patient bore, is wrapped around the entire circumference of the patient bore tube 1 and is firmly mounted to the patient bore tube 1. The large-volume rf coil, however, is subject to pulsed gradient fields from the gradient assembly 3. These pulsed fields induce eddy currents in the conductors of the large-volume rf coil and the eddy currents, in conjunction with the static magnetic field, produce $\vec{I} \times \vec{B}$ Lorentz forces which cause the patient bore tube 1 to vibrate. These vibrations then produce acoustic noise that can be heard by the patient and system operators.

[0023] In an embodiment of an imaging apparatus for producing MR images of a subject, the imaging apparatus comprises a gradient coil assembly, an rf coil assembly and the magnet assembly, and wherein each of the assemblies are selectively configured to reduce the generation and transmission of acoustic noise in and about the imaging apparatus during imaging. Each of the gradient assembly, rf coil assembly, the magnet assembly and other components of a MRI system contributes sources and pathways for acoustic noise. Embodiments are presented to reduce acoustic noise in each of the assemblies. It can be appreciated that for particular applications, features of each embodiment for the assemblies and components may be combined to lower acoustic noise of the imaging apparatus. Alternatively, each of the assemblies may be selectively configured to reduce the generation and transmission of acoustic noise independently. As used herein, "configured to" and the like refer to components having a structure and a capability for performing a stated function.

[0024] Gradient coil assembly 3 is desirably configured to reduce vibrations due to Lorentz forces acting on the gradient coils and vibrations due to electrically conductive parts not in contact with gradient coil assembly 3. Typically, the gradient coil assembly has two windings, inner and outer, which are held together by an epoxy filling. In a known manner, the epoxy filling stiffens and increases the weight of the gradient assembly in order to reduce the vibrations and resultant noise. In a first embodiment of gradient coil assembly 3, gradient coil assembly 3 is further mounted within the magnet assembly in a manner to provide further vibration isolation. Referring to Figure 1, each end of gradient assembly 3 is attached to a bracket 8 and a corresponding bracket 9 is attached to each corresponding end of the magnet. Disposed between brackets 8 and 9 are compliant isolation stacks 10, each having a thickness desirably between 3-10 mm. Compliant isolation stacks 10 provide vibration isolation between the gradient assembly and the magnet mounting the gradient assembly in way that reduces the vibration transmission from the gradient assembly to the magnet or other parts of the MRI system. In a further embodiment of gradient coil assembly 3, gradient coil assembly 3 is further contained in a vacuum 11 which is bounded by the patient bore tube 1, the magnet warm bore 4 and the end caps 12. In order to be effective for acoustic noise reduction, this

vacuum is desirably below 200 Torr.

[0025] Radiofrequency (rf) coil assembly 2 is desirably configured to reduce acoustic noise generated during imaging by alleviating the large-volume rf coil vibration and subsequent noise. Figures 4 and 5 show variations of embodiments of a reduced noise rf coil assembly 5
10
15
20
25
30
35
40
45
50
55
60
65
70
75
80
85
90
95
100
105
110
115
120
125
130
135
140
145
150
155
160
165
170
175
180
185
190
195
200
205
210
215
220
225
230
235
240
245
250
255
260
265
270
275
280
285
290
295
300
305
310
315
320
325
330
335
340
345
350
355
360
365
370
375
380
385
390
395
400
405
410
415
420
425
430
435
440
445
450
455
460
465
470
475
480
485
490
495
500
505
510
515
520
525
530
535
540
545
550
555
560
565
570
575
580
585
590
595
600
605
610
615
620
625
630
635
640
645
650
655
660
665
670
675
680
685
690
695
700
705
710
715
720
725
730
735
740
745
750
755
760
765
770
775
780
785
790
795
800
805
810
815
820
825
830
835
840
845
850
855
860
865
870
875
880
885
890
895
900
905
910
915
920
925
930
935
940
945
950
955
960
965
970
975
980
985
990
995
1000
1005
1010
1015
1020
1025
1030
1035
1040
1045
1050
1055
1060
1065
1070
1075
1080
1085
1090
1095
1100
1105
1110
1115
1120
1125
1130
1135
1140
1145
1150
1155
1160
1165
1170
1175
1180
1185
1190
1195
1200
1205
1210
1215
1220
1225
1230
1235
1240
1245
1250
1255
1260
1265
1270
1275
1280
1285
1290
1295
1300
1305
1310
1315
1320
1325
1330
1335
1340
1345
1350
1355
1360
1365
1370
1375
1380
1385
1390
1395
1400
1405
1410
1415
1420
1425
1430
1435
1440
1445
1450
1455
1460
1465
1470
1475
1480
1485
1490
1495
1500
1505
1510
1515
1520
1525
1530
1535
1540
1545
1550
1555
1560
1565
1570
1575
1580
1585
1590
1595
1600
1605
1610
1615
1620
1625
1630
1635
1640
1645
1650
1655
1660
1665
1670
1675
1680
1685
1690
1695
1700
1705
1710
1715
1720
1725
1730
1735
1740
1745
1750
1755
1760
1765
1770
1775
1780
1785
1790
1795
1800
1805
1810
1815
1820
1825
1830
1835
1840
1845
1850
1855
1860
1865
1870
1875
1880
1885
1890
1895
1900
1905
1910
1915
1920
1925
1930
1935
1940
1945
1950
1955
1960
1965
1970
1975
1980
1985
1990
1995
2000
2005
2010
2015
2020
2025
2030
2035
2040
2045
2050
2055
2060
2065
2070
2075
2080
2085
2090
2095
2100
2105
2110
2115
2120
2125
2130
2135
2140
2145
2150
2155
2160
2165
2170
2175
2180
2185
2190
2195
2200
2205
2210
2215
2220
2225
2230
2235
2240
2245
2250
2255
2260
2265
2270
2275
2280
2285
2290
2295
2300
2305
2310
2315
2320
2325
2330
2335
2340
2345
2350
2355
2360
2365
2370
2375
2380
2385
2390
2395
2400
2405
2410
2415
2420
2425
2430
2435
2440
2445
2450
2455
2460
2465
2470
2475
2480
2485
2490
2495
2500
2505
2510
2515
2520
2525
2530
2535
2540
2545
2550
2555
2560
2565
2570
2575
2580
2585
2590
2595
2600
2605
2610
2615
2620
2625
2630
2635
2640
2645
2650
2655
2660
2665
2670
2675
2680
2685
2690
2695
2700
2705
2710
2715
2720
2725
2730
2735
2740
2745
2750
2755
2760
2765
2770
2775
2780
2785
2790
2795
2800
2805
2810
2815
2820
2825
2830
2835
2840
2845
2850
2855
2860
2865
2870
2875
2880
2885
2890
2895
2900
2905
2910
2915
2920
2925
2930
2935
2940
2945
2950
2955
2960
2965
2970
2975
2980
2985
2990
2995
3000
3005
3010
3015
3020
3025
3030
3035
3040
3045
3050
3055
3060
3065
3070
3075
3080
3085
3090
3095
3100
3105
3110
3115
3120
3125
3130
3135
3140
3145
3150
3155
3160
3165
3170
3175
3180
3185
3190
3195
3200
3205
3210
3215
3220
3225
3230
3235
3240
3245
3250
3255
3260
3265
3270
3275
3280
3285
3290
3295
3300
3305
3310
3315
3320
3325
3330
3335
3340
3345
3350
3355
3360
3365
3370
3375
3380
3385
3390
3395
3400
3405
3410
3415
3420
3425
3430
3435
3440
3445
3450
3455
3460
3465
3470
3475
3480
3485
3490
3495
3500
3505
3510
3515
3520
3525
3530
3535
3540
3545
3550
3555
3560
3565
3570
3575
3580
3585
3590
3595
3600
3605
3610
3615
3620
3625
3630
3635
3640
3645
3650
3655
3660
3665
3670
3675
3680
3685
3690
3695
3700
3705
3710
3715
3720
3725
3730
3735
3740
3745
3750
3755
3760
3765
3770
3775
3780
3785
3790
3795
3800
3805
3810
3815
3820
3825
3830
3835
3840
3845
3850
3855
3860
3865
3870
3875
3880
3885
3890
3895
3900
3905
3910
3915
3920
3925
3930
3935
3940
3945
3950
3955
3960
3965
3970
3975
3980
3985
3990
3995
4000
4005
4010
4015
4020
4025
4030
4035
4040
4045
4050
4055
4060
4065
4070
4075
4080
4085
4090
4095
4100
4105
4110
4115
4120
4125
4130
4135
4140
4145
4150
4155
4160
4165
4170
4175
4180
4185
4190
4195
4200
4205
4210
4215
4220
4225
4230
4235
4240
4245
4250
4255
4260
4265
4270
4275
4280
4285
4290
4295
4300
4305
4310
4315
4320
4325
4330
4335
4340
4345
4350
4355
4360
4365
4370
4375
4380
4385
4390
4395
4400
4405
4410
4415
4420
4425
4430
4435
4440
4445
4450
4455
4460
4465
4470
4475
4480
4485
4490
4495
4500
4505
4510
4515
4520
4525
4530
4535
4540
4545
4550
4555
4560
4565
4570
4575
4580
4585
4590
4595
4600
4605
4610
4615
4620
4625
4630
4635
4640
4645
4650
4655
4660
4665
4670
4675
4680
4685
4690
4695
4700
4705
4710
4715
4720
4725
4730
4735
4740
4745
4750
4755
4760
4765
4770
4775
4780
4785
4790
4795
4800
4805
4810
4815
4820
4825
4830
4835
4840
4845
4850
4855
4860
4865
4870
4875
4880
4885
4890
4895
4900
4905
4910
4915
4920
4925
4930
4935
4940
4945
4950
4955
4960
4965
4970
4975
4980
4985
4990
4995
5000
5005
5010
5015
5020
5025
5030
5035
5040
5045
5050
5055
5060
5065
5070
5075
5080
5085
5090
5095
5100
5105
5110
5115
5120
5125
5130
5135
5140
5145
5150
5155
5160
5165
5170
5175
5180
5185
5190
5195
5200
5205
5210
5215
5220
5225
5230
5235
5240
5245
5250
5255
5260
5265
5270
5275
5280
5285
5290
5295
5300
5305
5310
5315
5320
5325
5330
5335
5340
5345
5350
5355
5360
5365
5370
5375
5380
5385
5390
5395
5400
5405
5410
5415
5420
5425
5430
5435
5440
5445
5450
5455
5460
5465
5470
5475
5480
5485
5490
5495
5500
5505
5510
5515
5520
5525
5530
5535
5540
5545
5550
5555
5560
5565
5570
5575
5580
5585
5590
5595
5600
5605
5610
5615
5620
5625
5630
5635
5640
5645
5650
5655
5660
5665
5670
5675
5680
5685
5690
5695
5700
5705
5710
5715
5720
5725
5730
5735
5740
5745
5750
5755
5760
5765
5770
5775
5780
5785
5790
5795
5800
5805
5810
5815
5820
5825
5830
5835
5840
5845
5850
5855
5860
5865
5870
5875
5880
5885
5890
5895
5900
5905
5910
5915
5920
5925
5930
5935
5940
5945
5950
5955
5960
5965
5970
5975
5980
5985
5990
5995
6000
6005
6010
6015
6020
6025
6030
6035
6040
6045
6050
6055
6060
6065
6070
6075
6080
6085
6090
6095
6100
6105
6110
6115
6120
6125
6130
6135
6140
6145
6150
6155
6160
6165
6170
6175
6180
6185
6190
6195
6200
6205
6210
6215
6220
6225
6230
6235
6240
6245
6250
6255
6260
6265
6270
6275
6280
6285
6290
6295
6300
6305
6310
6315
6320
6325
6330
6335
6340
6345
6350
6355
6360
6365
6370
6375
6380
6385
6390
6395
6400
6405
6410
6415
6420
6425
6430
6435
6440
6445
6450
6455
6460
6465
6470
6475
6480
6485
6490
6495
6500
6505
6510
6515
6520
6525
6530
6535
6540
6545
6550
6555
6560
6565
6570
6575
6580
6585
6590
6595
6600
6605
6610
6615
6620
6625
6630
6635
6640
6645
6650
6655
6660
6665
6670
6675
6680
6685
6690
6695
6700
6705
6710
6715
6720
6725
6730
6735
6740
6745
6750
6755
6760
6765
6770
6775
6780
6785
6790
6795
6800
6805
6810
6815
6820
6825
6830
6835
6840
6845
6850
6855
6860
6865
6870
6875
6880
6885
6890
6895
6900
6905
6910
6915
6920
6925
6930
6935
6940
6945
6950
6955
6960
6965
6970
6975
6980
6985
6990
6995
7000
7005
7010
7015
7020
7025
7030
7035
7040
7045
7050
7055
7060
7065
7070
7075
7080
7085
7090
7095
7100
7105
7110
7115
7120
7125
7130
7135
7140
7145
7150
7155
7160
7165
7170
7175
7180
7185
7190
7195
7200
7205
7210
7215
7220
7225
7230
7235
7240
7245
7250
7255
7260
7265
7270
7275
7280
7285
7290
7295
7300
7305
7310
7315
7320
7325
7330
7335
7340
7345
7350
7355
7360
7365
7370
7375
7380
7385
7390
7395
7400
7405
7410
7415
7420
7425
7430
7435
7440
7445
7450
7455
7460
7465
7470
7475
7480
7485
7490
7495
7500
7505
7510
7515
7520
7525
7530
7535
7540
7545
7550
7555
7560
7565
7570
7575
7580
7585
7590
7595
7600
7605
7610
7615
7620
7625
7630
7635
7640
7645
7650
7655
7660
7665
7670
7675
7680
7685
7690
7695
7700
7705
7710
7715
7720
7725
7730
7735
7740
7745
7750
7755
7760
7765
7770
7775
7780
7785
7790
7795
7800
7805
7810
7815
7820
7825
7830
7835
7840
7845
7850
7855
7860
7865
7870
7875
7880
7885
7890
7895
7900
7905
7910
7915
7920
7925
7930
7935
7940
7945
7950
7955
7960
7965
7970
7975
7980
7985
7990
7995
8000
8005
8010
8015
8020
8025
8030
8035
8040
8045
8050
8055
8060
8065
8070
8075
8080
8085
8090
8095
8100
8105
8110
8115
8120
8125
8130
8135
8140
8145
8150
8155
8160
8165
8170
8175
8180
8185
8190
8195
8200
8205
8210
8215
8220
8225
8230
8235
8240
8245
8250
8255
8260
8265
8270
8275
8280
8285
8290
8295
8300
8305
8310
8315
8320
8325
8330
8335
8340
8345
8350
8355
8360
8365
8370
8375
8380
8385
8390
8395
8400
8405
8410
8415
8420
8425
8430
8435
8440
8445
8450
8455
8460
8465
8470
8475
8480
8485
8490
8495
8500
8505
8510
8515
8520
8525
8530
8535
8540
8545
8550
8555
8560
8565
8570
8575
8580
8585
8590
8595
8600
8605
8610
8615
8620
8625
8630
8635
8640
8645
8650
8655
8660
8665
8670
8675
8680
8685
8690
8695
8700
8705
8710
8715
8720
8725
8730
8735
8740
8745
8750
8755
8760
8765
8770
8775
8780
8785
8790
8795
8800
8805
8810
8815
8820
8825
8830
8835
8840
8845
8850
8855
8860
8865
8870
8875
8880
8885
8890
8895
8900
8905
8910
8915
8920
8925
8930
8935
8940
8945
8950
8955
8960
8965
8970
8975
8980
8985
8990
8995
9000
9005
9010
9015
9020
9025
9030
9035
9040
9045
9050
9055
9060
9065
9070
9075
9080
9085
9090
9095
9100
9105
9110
9115
9120
9125
9130
9135
9140
9145
9150
9155
9160
9165
9170
9175
9180
9185
9190
9195
9200
9205
9210
9215
9220
9225
9230
9235
9240
9245
9250
9255
9260
9265
9270
9275
9280
9285
9290
9295
9300
9305
9310
9315
9320
9325
9330
9335
9340
9345
9350
9355
9360
9365
9370
9375
9380
9385
9390
9395
9400
9405
9410
9415
9420
9425
9430
9435
9440
9445
9450
9455
9460
9465
9470
9475
9480
9485
9490
9495
9500
9505
9510
9515
9520
9525
9530
9535
9540
9545
9550
9555
9560
9565
9570
9575
9580
9585
9590
9595
9600
9605
9610
9615
9620
9625
9630
9635
9640
9645
9650
9655
9660
9665
9670
9675
9680
9685
9690
9695
9700
9705
9710
9715
9720
9725
9730
9735
9740
9745
9750
9755
9760
9765
9770
9775
9780
9785
9790
9795
9800
9805
9810
9815
9820
9825
9830
9835
9840
9845
9850
9855
9860
9865
9870
9875
9880
9885
9890
9895
9900
9905
9910
9915
9920
9925
9930
9935
9940
9945
9950
9955
9960
9965
9970
9975
9980
9985
9990
9995
10000
10005
10010
10015
10020
10025
10030
10035
10040
10045
10050
10055
10060
10065
10070
10075
10080
10085
10090
10095
10100
10105
10110
10115
10120
10125
10130
10135
10140
10145
10150
10155
10160
10165
10170
10175
10180
10185
10190
10195
10200
10205
10210
10215
10220
10225
10230
10235
10240
10245
10250
10255
10260

configured to reduce generation and transmission of acoustic noise. In one embodiment, magnet warm bore 4 is desirably made of non-electrically conductive material, for example, FRP (fiberglass-reinforced plastic). In a further embodiment, a vacuum surrounding the magnet warm bore prevents sound from being carried from the magnet warm bore by means of air. The seal between the magnet warm bore and the rest of the magnet structure can be made to carry out vibration isolation as well as a vacuum seal. If the seal can vibrationally isolate the warm bore from the rest of the magnet structure, then vibrations induced in the warm bore by gradient magnetic field pulses will not be carried mechanically to the outside of the cryostat shell 7. Thus, isolating the magnet warm bore via vacuum plus isolating the magnet warm bore by mechanical isolation can desirably prevent or decrease the ability of vibrations of the warm bore to produce acoustic noise which would be audible to the patient or MRI system operator. In another further embodiment the FRP is desirably coated with a very thin (microns or submicrons thick) metallic layer (metallized) in order to decrease penetration of gases and water from the atmosphere through the surface of the warm bore. If the metallic layer is made sufficiently thin (microns or submicrons thick), then eddy currents will be substantially minimized in the metallic layers and so will consequent eddy-current-induced vibrations.

[0033] Referring further to Figure 2, a further embodiment of the magnet assembly comprises suspension members 13 configured to reduce transmission of acoustic noise. Magnet vessel 6 is connected to cryostat shell 7 by thin suspension members 13. These members are typically designed to minimize heat flow from cryostat shell 7 to magnet vessel 6, including the superconducting magnet. In this embodiment, suspension members 13 are constructed to desirably vibrationally isolate magnet vessel 6 from cryostat shell 7. In this embodiment, suspension member 13 comprises a blocking mass 15 attached to the middle of suspension straps 14. Blocking mass 15 is made of electrically non-conducting material. Straps 14 can be constructed of carbon fiber material, as is well known. Transmission of high frequencies along suspension members 13 is desirably reduced by attaching mass 15 to the middle of the suspension members, thus creating a vibrational impedance mismatch that will tend to reflect energy traveling along the suspension members.

[0034] Further embodiments of the magnet assembly include embodiments of cryostat shell 7 that reduce acoustic noise attributable to the cryostat shell. The cryostat shell is generally metallic, typically steel or stainless steel. Vibrations of the cryostat shell, whether as a direct electromagnetic excitation from the pulsed gradient magnetic fields or as a result of mechanically transmitted vibrations originating somewhere else in the apparatus, can result in acoustic noise that is heard by the patient or MRI system operator.

[0035] In a further embodiment, cryostat shell 7 is de-

sirably made of non-electrically-conductive materials such as FRP. In another further embodiment the FRP is desirably coated with a very thin (microns or submicrons thick) metallic layer (metallized) in order to decrease penetration of gases and water from the atmosphere through the cryostat shell. If the metallic layer is made sufficiently thin (microns or submicrons thick), then eddy currents will be substantially minimized in the metallic layers and so will consequent eddy-current-induced vibrations.

[0036] Referring further to Figure 2, in a further embodiment, cryostat shell 7 is covered by a layer 17 of acoustic material which blocks and absorbs potential vibrations thus preventing acoustic noise emissions to the room and patient bore tube 1. Layer 17 is a material such as open-cell foam designed for acoustic absorption such as "Soundfoam" by Soundcoat Company, and in this embodiment is approximately 6 mm to 13 mm in thickness. Further disposed between layer 17 and cryostat shell is a layer of constrained-layer-damping (CLD) desirably applied as strips to the cryostat shell. CLD generally consists of a thin plate with an acoustically damping material applied to it. The CLD material is applied to the structure to be damped (cryostat shell 7) so that the damping material is sandwiched between the thin plate and the structure. As vibrations are conveyed through the structure, the structure flexes, and the consequent shear between the structure and the thin plate produces damping in the sandwiched acoustic damping material. This material can be effective in removing the effects of mechanical resonances, which often tend to increase sound levels. In another further embodiment, CLD material 100 is applied to the inner surface of warm bore 4. In another further embodiment, CLD material 100 is applied to the inner and/or outer surfaces of gradient assembly 3.

[0037] Further alternate embodiments of the magnet assembly involve mounting arrangements to prevent vibrations and resulting acoustic noise. For example, vibrations of the cryostat shell can also be conveyed to the patient bore tube via the mechanical path from cryostat shell 7 to end caps 12 to patient bore tube 1. In an embodiment for mounting the magnet assembly, the mechanical path is desirably broken up by ensuring that seals 20 between end caps 12 and cryostat shell 7, which maintains the vacuum around the gradient assembly, also serves as vibration isolation. In this embodiment, vibrations from the cryostat will be prevented from being transmitted to the patient bore tube. Seals 20 are selected to provide isolation between cryostat shell 7 and end caps 12. An embodiment includes seals 20 made of O-ring material such as Durometer 40 Buna-N rubber or other such materials.

[0038] Referring further to Figure 2, in a further embodiment, patient bore tube 1 includes a layer of acoustic absorptive material, such as "Soundfoam" disposed on its inner surface. Patient bore tube is typically made of a rigid, electrically low- or non-conducting material

such as FRP (fiberglass-reinforced plastic). Patient bore tube 1 may have mechanical resonances that would tend to amplify vibrations conveyed to the patient tube via mechanical contact or air. In a further embodiment, damping can be introduced to the patient tube resonances by applying non-conducting constrained-layer damping (CLD) 100 as in strips to the outer or inner surface of patient bore tube 1.

[0039] Referring to Figure 6, there is shown a further embodiment for reducing a source of acoustic noise due to the leads that power the gradient coils. The leads that power the gradient coils carry large currents, typically 200 A or more and may therefore be subjected to large Lorentz forces. Referring to Figure 1, leads or wires (not shown) pass through one of end caps 12 via gradient feed-through assembly 600. These leads must go from an external power supply to the gradient assembly and therefore must penetrate the vacuum enclosure. The large Lorentz forces on the gradient leads undesirably cause the wires to vibrate. If the gradient lead feed-through assemblies are rigidly attached to end caps 12, the forces on the gradient leads may cause the end caps to vibrate. This is undesirable since vibration of the relatively large-area end caps may then move a large volume of air and create a high-intensity sound.

[0040] Referring further to Figure 6, gradient feed-through assembly 600 is constructed to alleviate the problem of transferring vibrations to end caps 12. In this embodiment, clearance hole 602 is provided on end cap wall 601 to allow for power from an external power supply to pass through end cap wall 601. Threaded rod 603 goes through clearance hole 602 and rubber disks 604, and threaded rod 603 serves as a conductor for the current that is passed from wires 608 attached through lugs 607. Thus, wires 608, lugs 607 and threaded rod 603 serve as the conduction path for the power. Further, washers 605 and nuts 606 are provided to secure feed-through assembly 600 to the surface end cap wall 601, and nuts 606 also serve as part of the conduction path. Adjacent to each side of end cap wall 601 is pair of isolation devices 604, made of an electrically insulating material such as, for example, soft, tightly-fitting rubber spacers. Desirably, the rubber isolating material enables the feed-through assembly to have a small range of motion, in and out and tilting, thereby reducing vibration and subsequent acoustic noise. Also, isolation devices 604 also serve to produce an airtight seal in order to maintain the vacuum.

[0041] Referring to Figure 3, a further source and pathway of acoustic noise can be attributed to cradle electronics unit 300, the electronics unit used to interface the signals from various rf coils to the system electronics which are typically located external to the scanner. Typically, cradle electronics unit 300 contains electronic modules with metal parts that in turn may produce eddy currents when subjected to the pulsed imaging gradients, and these eddy currents may cause vibration and consequent sound generation. Some typical elec-

tronic modules might be preamplifiers or other electronic circuits contained in metal boxes, typically with dimensions of about 50 mm or larger. If these electronics are rigidly bolted onto some electronics-carrying carriage that is attached to patient couch 104 or is otherwise introduced into the imaging volume during imaging, then vibrations of the electronics may vibrate the cradle or couch. Since the cradle may have relatively large surface area, its vibration may efficiently produce acoustic sound. Therefore it is desirable to vibrationally isolate the electronics and to prevent any sound from the electronics from reaching the patient or system operator.

[0042] In a further embodiment, it is desirable to isolate the electronic modules in unit 300 by placing them on vibration absorbing or isolating material such as rubber pads inside unit 300, so that the rubber tends to prevent vibrations of the electronics from reaching the carriage. Additionally, sound-absorbing material, such as closed-cell acoustic foam or fiberglass batting, may be wrapped around the control unit 300.

[0043] For completeness, various aspects of the invention are set out in the following numbered clauses:

1. An imaging apparatus for producing Magnetic Resonance (MR) images of a subject (200) contained within a patient bore tube defining an imaging volume (101) and for substantially minimizing acoustic noise generated during imaging, said apparatus comprising:

a magnet assembly (4,6,7) for producing a static magnetic field;
a gradient coil assembly (3) disposed within said magnet assembly for generating a magnetic field gradient for use in producing MR images; and,
a radiofrequency (rf) coil assembly (2) contained between said gradient coil assembly and said patient bore tube for transmitting a radiofrequency pulse and for receiving an MR signal induced from said subject;

wherein at least one of said magnet assembly, said gradient coil assembly and said rf coil assembly is selectively configured to reduce generation and transmission of acoustic noise.

2. The imaging apparatus of clause 1 wherein said magnet coil assembly (4,6,7), said gradient coil assembly and said rf coil assembly are each generally annularly, cylindrically shaped:

3. The imaging apparatus of clause 1 wherein said gradient coil assembly (3) is disposed within a vacuum enclosure (11) within said magnet assembly, said vacuum being between about .1 and about 200 Torr.

4. The imaging apparatus of clause 1 further comprising at least one isolation mounting device (10) for mounting said gradient coil assembly (3) within said magnet assembly (4,6,7) and for reducing acoustic noise due to vibration transmission. 5
5. The imaging apparatus of clause 1 further comprising subject support structures (102,104,105,106) for guiding and supporting said subject (200) within said imaging volume, wherein at least one of an inner surface of said patient bore tube (1) and said subject support structures is constructed to include a layer of an acoustic absorptive material. 10
6. The imaging apparatus of clause 1 wherein an inner surface (4) of said magnet assembly comprises a non-conducting material. 15
7. The imaging apparatus of clause 1 wherein an outer surface (7) of said magnet assembly comprises a non-conducting material. 20
8. The imaging apparatus of clause 1 wherein an outer surface (7) of said magnet assembly comprises a non-conducting material having a thin metallic layer to prevent penetration of air and water vapor from the atmosphere. 25
9. The imaging apparatus of clause 1 wherein said rf coil assembly (2) comprises: 30
- a plurality of conductors (402,502) for transmitting a radiofrequency pulse, for receiving an MR signal induced in said subject (200), said conductors having respective widths selected for reducing eddy current excitation contributing to acoustic noise. 35
10. The imaging apparatus of clause 9 wherein said conductors (502) comprise Cu tubing having an outside diameter of approximately 3mm to 12mm. 40
11. The imaging apparatus of clause 9 wherein said conductors (402) comprise Cu strips and said respective width is less than approximately 50 mm. 45
12. The imaging apparatus of clause 1 wherein said rf coil assembly (2) comprises: 50
- a plurality of conductors (502) for transmitting a radiofrequency pulse and for receiving an MR signal induced in said subject, said conductors having respective widths selected for reducing eddy current excitation contributing to acoustic noise in and about said imaging apparatus; and, 55
- a layer of vibration isolation material (504) disposed between said plurality of conductors (502) and said patient bore tube (1).
13. The imaging apparatus of clause 12 wherein said conductors (502) comprise tubing having an outside diameter of approximately 3mm to 12mm.
14. The imaging apparatus of clause 13 further comprising a plurality of straps (505) to hold said conductors and said layer of vibration isolation material (504) fixably on said patient bore tube (1).
15. The imaging apparatus of clause 1 wherein said magnet assembly further comprises passive magnet shims (5) fixed on an inner surface (4) of said magnet assembly for adjusting said static magnetic field and said passive shims comprise a non-conducting material.
16. The imaging apparatus of clause 1 wherein said magnet assembly further comprises passive shim magnets (6) fixed on an inner surface (4) of said magnet assembly for adjusting said static magnetic field, said passive shims being constructed of respective layers of a non-conducting material and cushioning material.
17. The imaging apparatus of clause 1 wherein said patient bore tube (1) is constructed of a non-conducting material.
18. The imaging apparatus of clause 1 wherein an inner surface (4) of said patient bore tube comprises a layer of acoustic absorptive material.
19. The imaging apparatus of clause 1 further comprising a pair of end caps (12) for mounting respective ends of said patient bore tube (1) to respective ends of said magnet assembly (4,6,7).
20. The imaging apparatus of clause 19 further comprising end caps seals (20) disposed between said end caps (12) to said respective ends of said patient bore tube (1) and said magnet assembly (4,6,7).
21. The imaging apparatus of clause 19 wherein a sealed gap is disposed between said end caps (12) and said respective ends of said patient bore tube (1) and said magnet assembly (4,6,7).
22. The imaging apparatus of clause 1 wherein said rf coil assembly (2) is mounted so that it has a spaced apart relationship with said patient bore tube (1).
23. The imaging apparatus of clause 1 wherein said gradient coil assembly (3) further comprises a vi-

bration isolating feed-through assembly (600) for gradient leads from an external power supply.

24. The imaging apparatus of clause 1 wherein said magnet assembly further comprises constrained-layer damping material (16) disposed about at least one of an inner (4) or an outer surface (7) of said magnet assembly.

25. The imaging apparatus of clause 1 further comprising constrained-layer damping material (100) disposed about at least one of an outer surface or inner surface of said patient bore tube (1).

26. The imaging apparatus of clause 5 further comprising an electronics unit (300) for interfacing between said rf coil assembly (2) and external system electronics, said electronics unit being constructed to reduce acoustic noise.

27. The imaging apparatus of clause 1 wherein an inner surface (4) of said magnet assembly comprises a non-conducting material having a thin metallic layer to prevent penetration of air and water vapor from the atmosphere.

28. An imaging apparatus for producing Magnetic Resonance (MR) images of a subject (200) contained in a patient bore tube (1) defining an imaging volume (101) and for substantially minimizing acoustic noise generated during imaging, said imaging apparatus comprising:

a magnet assembly (4,6,7) for producing a static magnetic field having an inner surface (4) of non-conducting material (7) and an outer surface of acoustic absorptive material (17); a gradient coil assembly (3) disposed within a vacuum enclosure (11) within said magnet assembly for generating a magnetic field gradient for use in producing MR images, said gradient coil being mounted within said magnet assembly with at least one isolation mounting device (10) to reduce vibration transmission between said gradient coil assembly and said magnet assembly; an rf coil assembly (2) disposed about an outer surface of said patient bore tube (1) and contained within said gradient coil assembly (3) for transmitting a radiofrequency pulse and for receiving an MR signal induced from said subject (200), respective ends of said rf coil assembly being mounted to respective ends of said magnet assembly to reduce generation and transmission of acoustic noise between said rf coil assembly and said magnet assembly; and, support structures (102,104,105,106) for guiding and supporting said subject (200) into said

imaging volume (101), said support structures being configured to reduce generation and transmission of acoustic noise.

29. The imaging apparatus of clause 28 wherein said magnet assembly, said gradient coil assembly and said rf coil assembly form a generally annular and cylindrical structure.

30. The imaging apparatus of clause 28 wherein said wherein at least one of an inner surface of said patient bore tube (1) and said subject support structures is constructed to include a layer of an acoustic absorptive material.

31. The imaging apparatus of clause 28 wherein said magnet (5) assembly further comprises passive shim magnets fixed on an inner surface (4) of said magnet assembly adapted for adjusting said static magnetic field and said passive shims are constructive of a non-conducting material.

32. The imaging apparatus of clause 28 wherein said magnet assembly further comprises passive shim magnets (5) fixed on an inner surface (4) of said magnet assembly for adjusting said static magnetic field, said passive shims being constructive of respective layers of a non-conducting material and cushioning material.

33. The imaging apparatus of clause 28 further comprising constrained-layer damping material (100) disposed about at least one of an outer or an inner surface of said patient bore tube (1) and at least one of an outer (7) or an inner surface (4) of said magnet assembly to damp vibrations.

34. The imaging apparatus of clause 28 wherein said gradient coil assembly (3) further comprises a vibration isolating feed-through assembly (600) for gradient leads from an external power supply.

35. A magnet assembly for an imaging apparatus for a Magnetic Resonance Imaging (MRI) system, wherein said system is provided with a generally annular and cylindrical main magnet for generating a static magnetic field, a gradient coil assembly (3) located within an inner surface (4) of said magnet for generating magnetic field gradient for use in producing MR images, and a rf coil assembly (2) disposed within said gradient coil assembly for transmitting a radiofrequency pulse and for receiving an MR signal induced from a subject (200) to be imaged in said imaging apparatus, said magnet assembly comprising:

an outer surface (7); and,
a plurality suspension members (13) for attach-

ing said magnet to said outer surface, said suspension members being configured to reduce generation and transmission of acoustic noise.

36. The magnet assembly of clause 35 further wherein said suspension members (13) each comprise a blocking mass (15) attached to a suspension strap (14) for isolating vibration of the magnet assembly.

37. The magnet assembly of clause 35 wherein said outer surface (7) comprises a non-conducting material.

38. A rf coil assembly for an imaging apparatus for a Magnetic Resonance Imaging (MRI) system, wherein said system is provided with a generally annular and cylindrical main magnet for generating a static magnetic field, a gradient coil assembly (3) located within an inner surface (4) of said magnet for generating magnetic field gradient for use in producing MR images, and said rf coil assembly is disposed within said gradient coil assembly for transmitting a radiofrequency pulse and for receiving an MR signal induced from a subject to be imaged in an imaging volume (101) of said imaging apparatus, said rf coil assembly comprising:

a plurality of conductors (502) having a width selected for transmitting a radiofrequency pulse, for receiving an MR signal induced in said subject and for reducing eddy current excitation contributing to acoustic noise in and about said imaging apparatus; and, a layer of vibration isolation material (504) disposed between said plurality of conductors and a patient bore tube, said patient bore tube (1) being for receiving said subject into said imaging volume (101).

39. The rf coil assembly of clause 38 wherein said plurality of conductors (54) are constructed of Cu tubing having an outside diameter of approximately 3mm to 12mm.

40. The rf coil assembly of clause 38 wherein said conductors (502) are constructed of Cu strips and said width is less than approximately 5mm.

41. The rf coil assembly of clause 38 further comprising a plurality of straps (505) to hold said conductors (502) and said layer of vibration isolation material (504) fixably on said patient bore tube (1).

42. The imaging apparatus of clause 1 wherein said magnet assembly is an open magnet.

Claims

1. An imaging apparatus for producing Magnetic Resonance (MR) images of a subject (200) contained within a patient bore tube defining an imaging volume (101) and for substantially minimizing acoustic noise generated during imaging, said apparatus comprising:

a magnet assembly (4,6,7) for producing a static magnetic field;

a gradient coil assembly (3) disposed within said magnet assembly for generating a magnetic field gradient for use in producing MR images; and,

a radiofrequency (rf) coil assembly (2) contained between said gradient coil assembly and said patient bore tube for transmitting a radiofrequency pulse and for receiving an MR signal induced from said subject;

wherein at least one of said magnet assembly, said gradient coil assembly and said rf coil assembly is selectively configured to reduce generation and transmission of acoustic noise.

2. The imaging apparatus of claim 1 further comprising at least one isolation mounting device (10) for mounting said gradient coil assembly (3) within said magnet assembly (4,6,7) and for reducing acoustic noise due to vibration transmission.

3. The imaging apparatus of claim 1 further comprising subject support structures (102,104,105,106) for guiding and supporting said subject (200) within said imaging volume, wherein at least one of an inner surface of said patient bore tube (1) and said subject support structures is constructed to include a layer of a acoustic absorptive material.

4. The imaging apparatus of claim 1 wherein said rf coil assembly (2) comprises:

a plurality of conductors (402,502) for transmitting a radiofrequency pulse, for receiving an MR signal induced in said subject (200), said conductors having respective widths selected for reducing eddy current excitation contributing to acoustic noise.

5. An imaging apparatus for producing Magnetic Resonance (MR) images of a subject (200) contained in a patient bore tube (1) defining an imaging volume (101) and for substantially minimizing acoustic noise generated during imaging, said imaging apparatus comprising:

a magnet assembly (4,6,7) for producing a static

- ic magnetic field having an inner surface (4) of non-conducting material (7) and an outer surface of acoustic absorptive material (17); a gradient coil assembly (3) disposed within a vacuum enclosure (11) within said magnet assembly for generating a magnetic field gradient for use in producing MR images, said gradient coil being mounted within said magnet assembly with at least one isolation mounting device (10) to reduce vibration transmission between said gradient coil assembly and said magnet assembly;
- an rf coil assembly (2) disposed about an outer surface of said patient bore tube (1) and contained within said gradient coil assembly (3) for transmitting a radiofrequency pulse and for receiving an MR signal induced from said subject (200), respective ends of said rf coil assembly being mounted to respective ends of said magnet assembly to reduce generation and transmission of acoustic noise between said rf coil assembly and said magnet assembly; and, support structures (102,104,105,106) for guiding and supporting said subject (200) into said imaging volume (101), said support structures being configured to reduce generation and transmission of acoustic noise.
6. The imaging apparatus of claim 5 wherein said wherein at least one of an inner surface of said patient bore tube (1) and said subject support structures is constructed to include a layer of an acoustic absorptive material.
7. The imaging apparatus of claim 5 wherein said magnet assembly further comprises passive shim magnets (5) fixed on an inner surface (4) of said magnet assembly for adjusting said static magnetic field, said passive shims being constructive of respective layers of a non-conducting material and cushioning material.
8. A magnet assembly for an imaging apparatus for a Magnetic Resonance Imaging (MRI) system, wherein said system is provided with a generally annular and cylindrical main magnet for generating a static magnetic field, a gradient coil assembly (3) located within an inner surface (4) of said magnet for generating magnetic field gradient for use in producing MR images, and a rf coil assembly (2) disposed within said gradient coil assembly for transmitting a radiofrequency pulse and for receiving an MR signal induced from a subject (200) to be imaged in said imaging apparatus, said magnet assembly comprising:
- an outer surface (7); and,
a plurality suspension members (13) for attaching said magnet to said outer surface, said suspension members being configured to reduce generation and transmission of acoustic noise.
9. The magnet assembly of claim 8 further wherein said suspension members (13) each comprise a blocking mass (15) attached to a suspension strap (14) for isolating vibration of the magnet assembly.
10. A rf coil assembly for an imaging apparatus for a Magnetic Resonance Imaging (MRI) system, wherein said system is provided with a generally annular and cylindrical main magnet for generating a static magnetic field, a gradient coil assembly (3) located within an inner surface (4) of said magnet for generating magnetic field gradient for use in producing MR images, and said rf coil assembly is disposed within said gradient coil assembly for transmitting a radiofrequency pulse and for receiving an MR signal induced from a subject to be imaged in an imaging volume (101) of said imaging apparatus, said rf coil assembly comprising:
- a plurality of conductors (502) having a width selected for transmitting a radiofrequency pulse, for receiving an MR signal induced in said subject and for reducing eddy current excitation contributing to acoustic noise in and about said imaging apparatus; and,
a layer of vibration isolation material (504) disposed between said plurality of conductors and a patient bore tube, said patient bore tube (1) being for receiving said subject into said imaging volume (101).

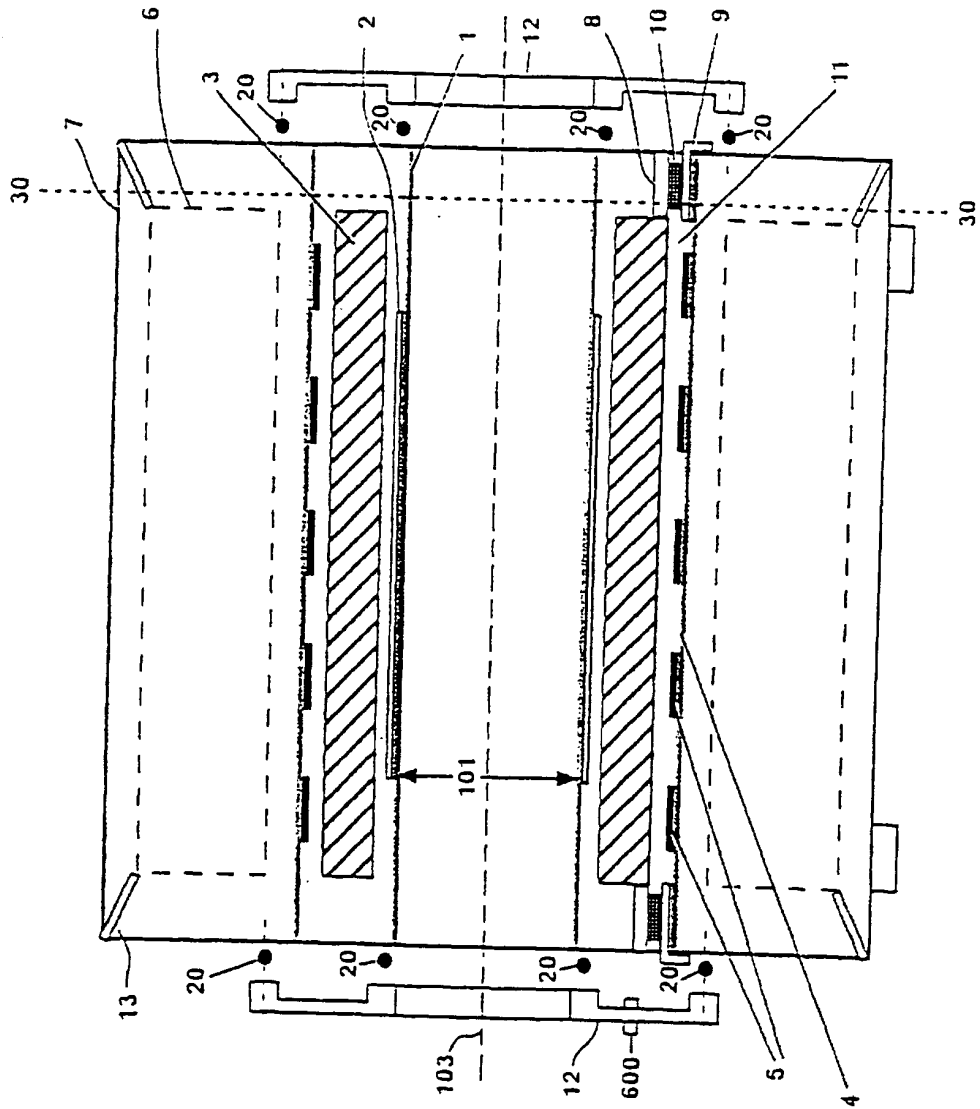


Fig. 1

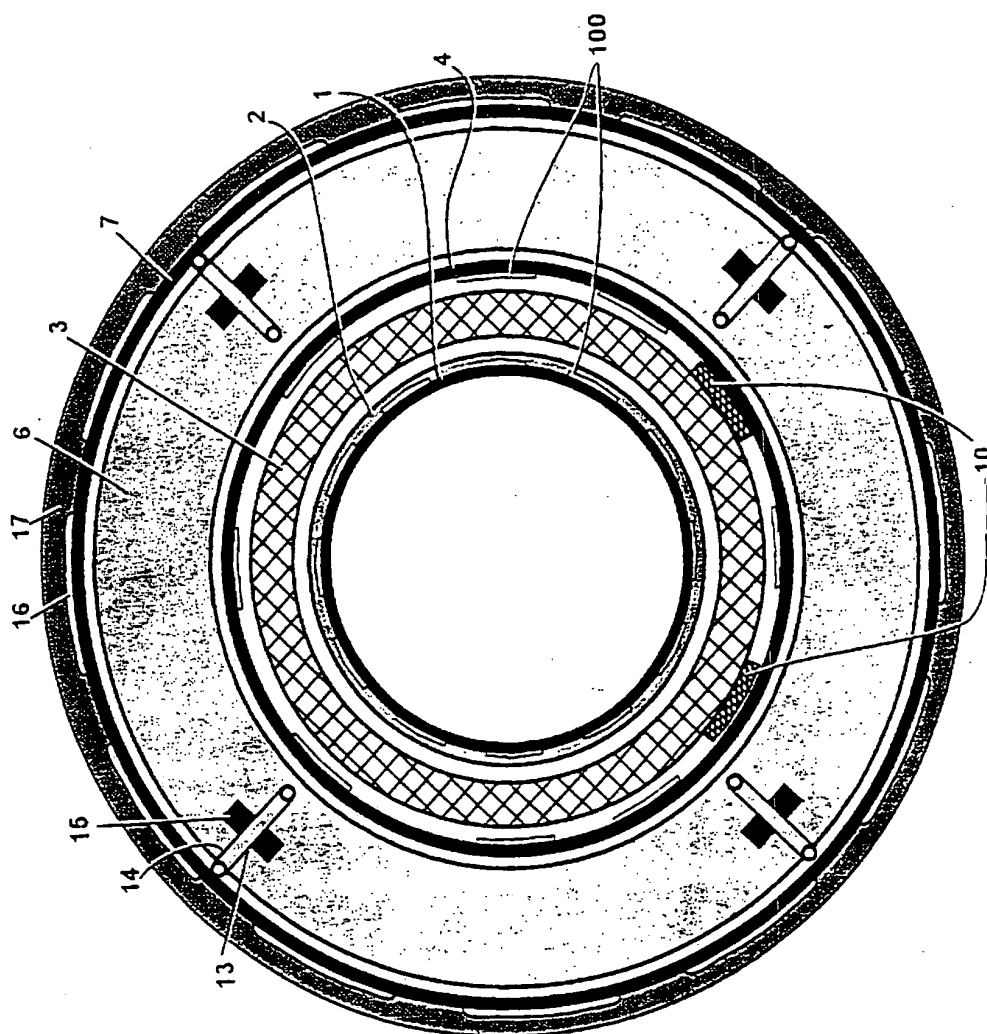


Fig. 2

BEST AVAILABLE COP



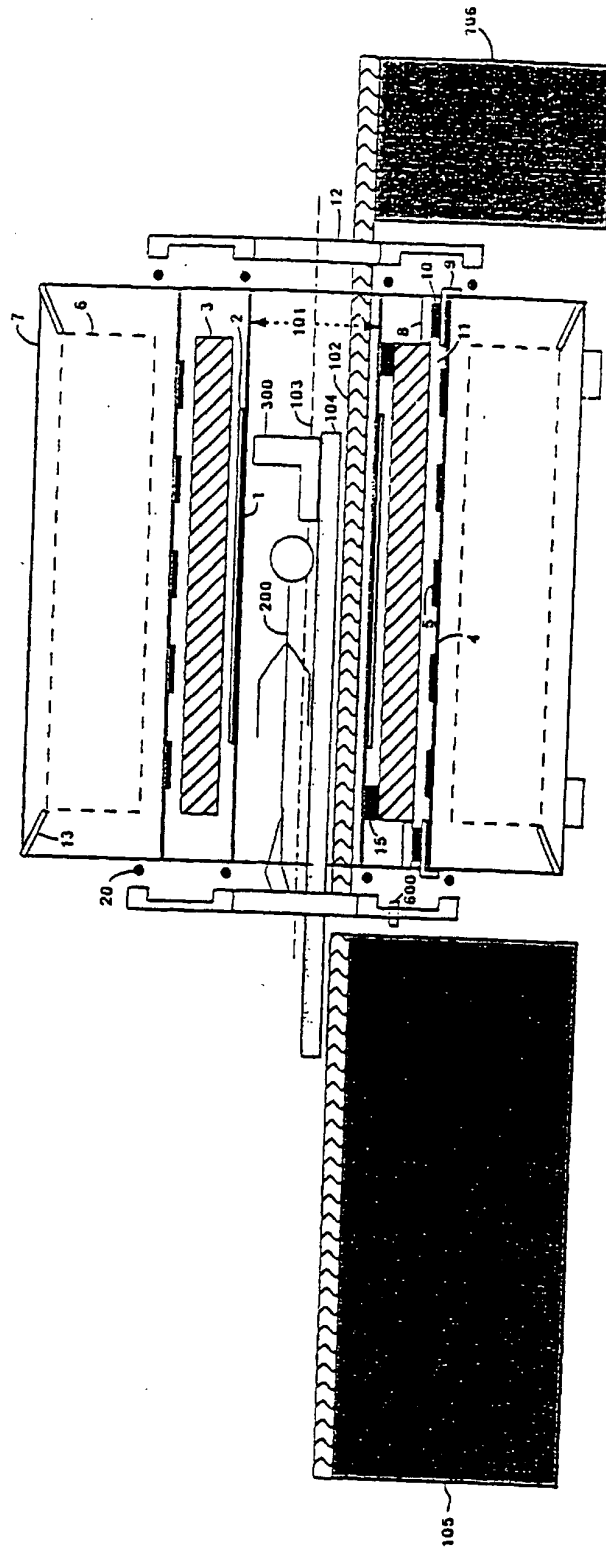


Fig. 3

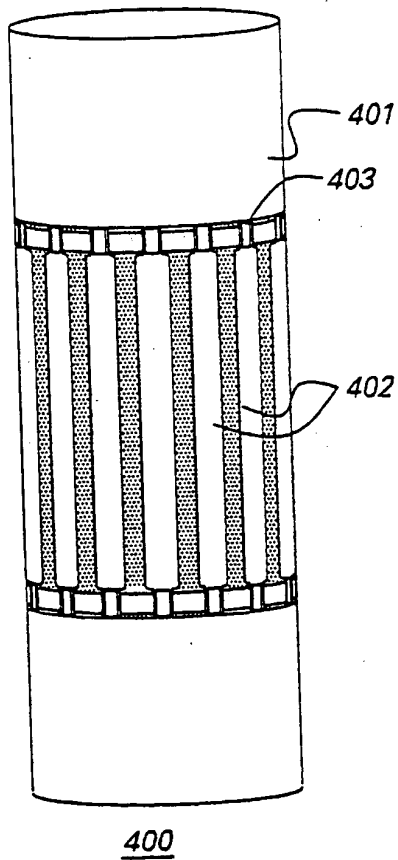

400
fig. 4

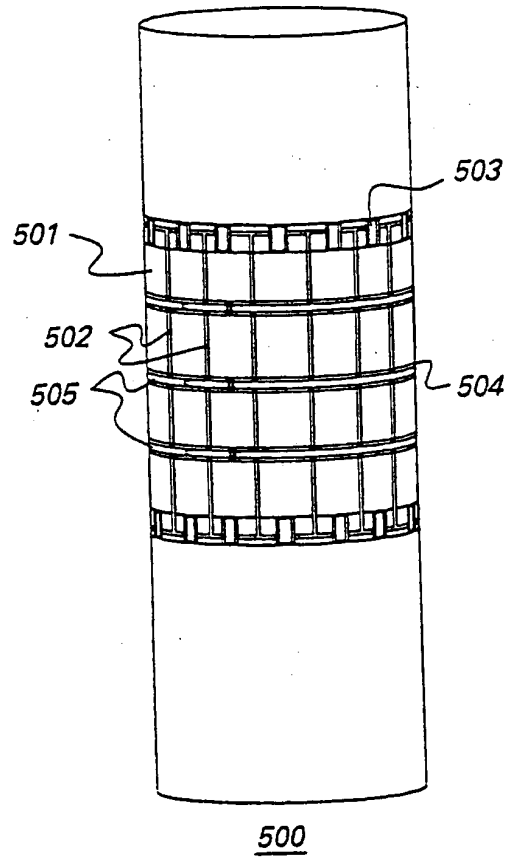

500
fig. 5

BEST AVAILABLE COPY

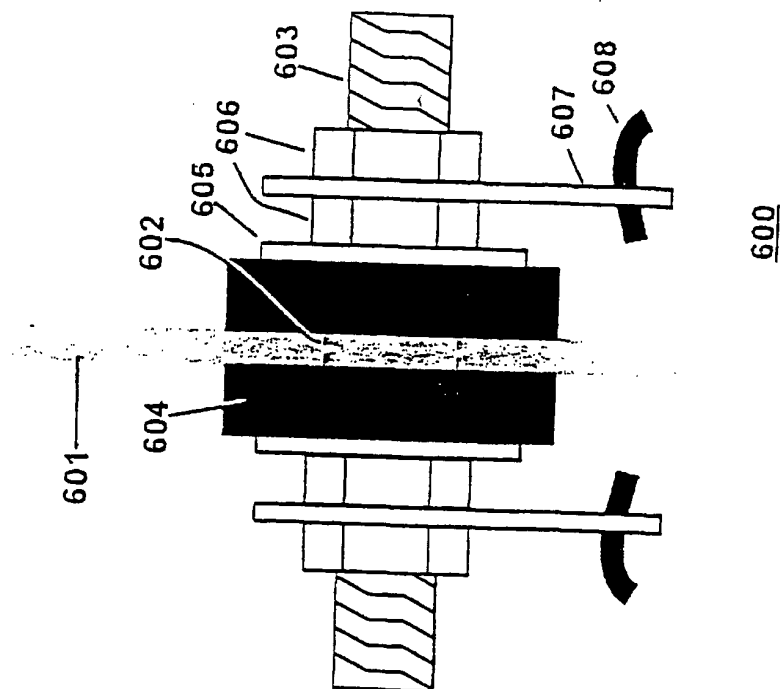


Fig. 6